


TRIAL OF EARLY, GOAL-DIRECTED RESUSCITATION FOR SEPTIC SHOCK

The ProMISe Trial

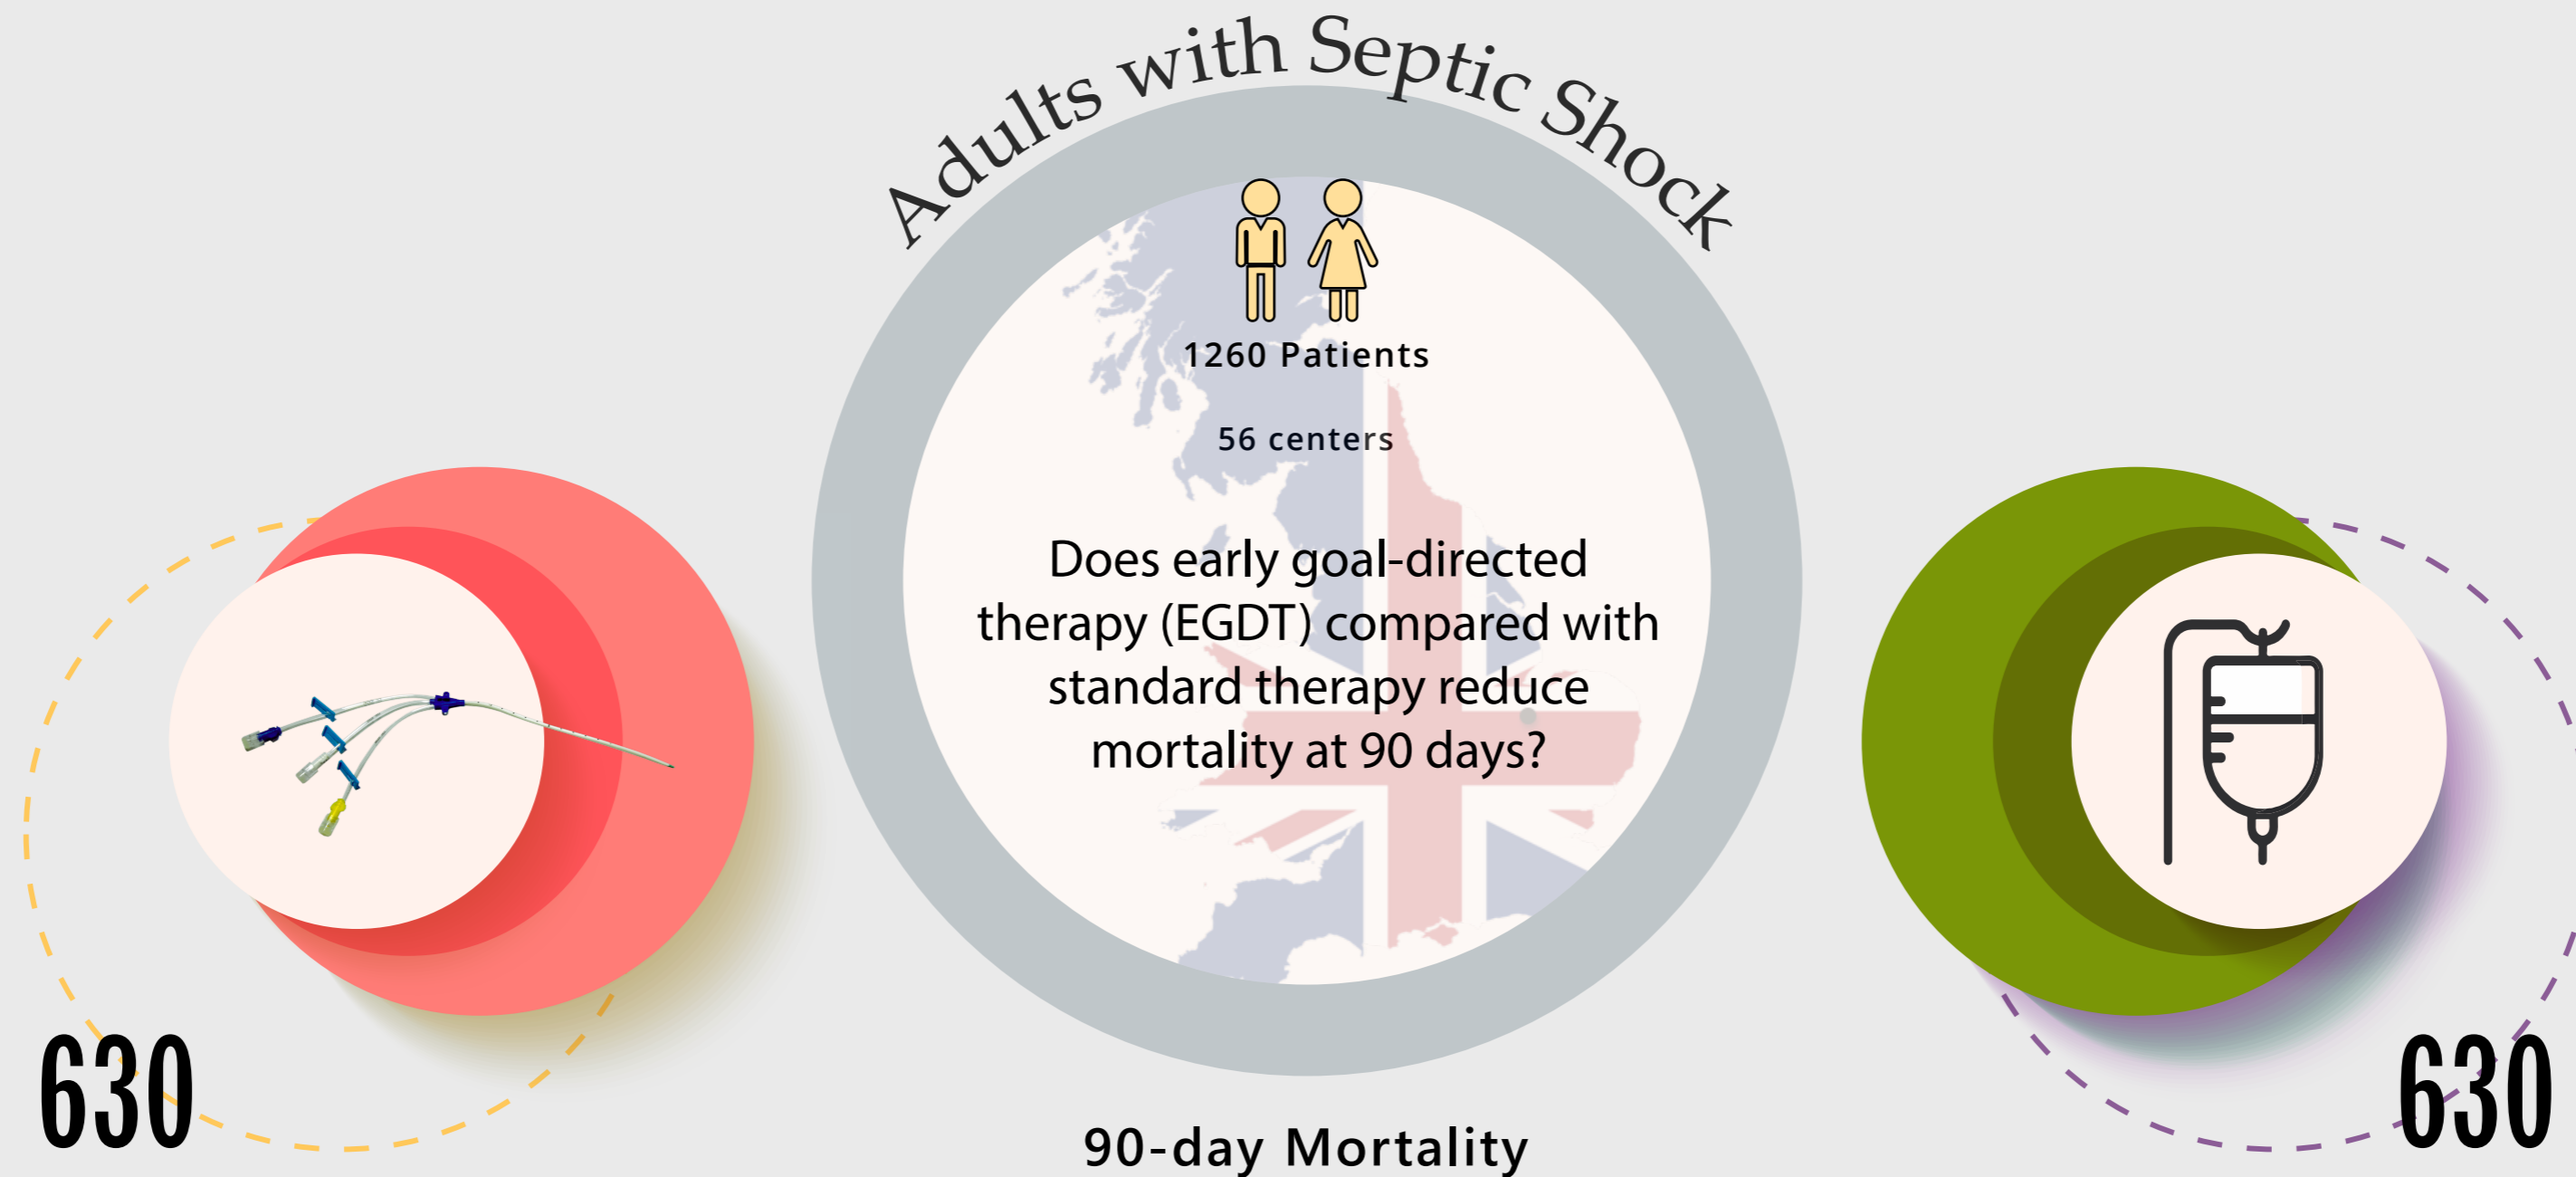

EGDT

Central venous catheter capable of continuous ScvO₂ monitoring was placed in 87%.
Data were collected prospectively.

USUAL CARE

51% had central line as part of the usual care.
Data were collected retrospectively.

A strict EGDT protocol in patients with septic shock who were resuscitated and received intravenous antibiotics, did not lead to an improvement in outcome

April 2, 2015